


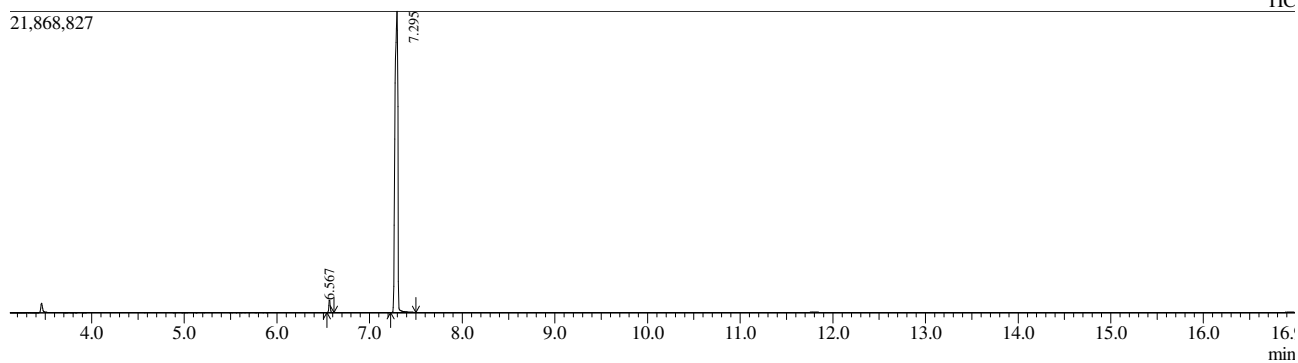


Peak#	R.Time	I.Time	F.Time	Area	Area%	Height	Height%	A/H	Mark	Name
1	6.567	6.540	6.615	960954	1.99	882082	3.88	1.09	MI	
2	7.295	7.225	7.500	47392923	98.01	21829067	96.12	2.17	MI	
				48353877	100.00	22711149	100.00			

Spectrum


Peak#:1 R.Time:6.567(Scan#:694)

MassPeaks:284

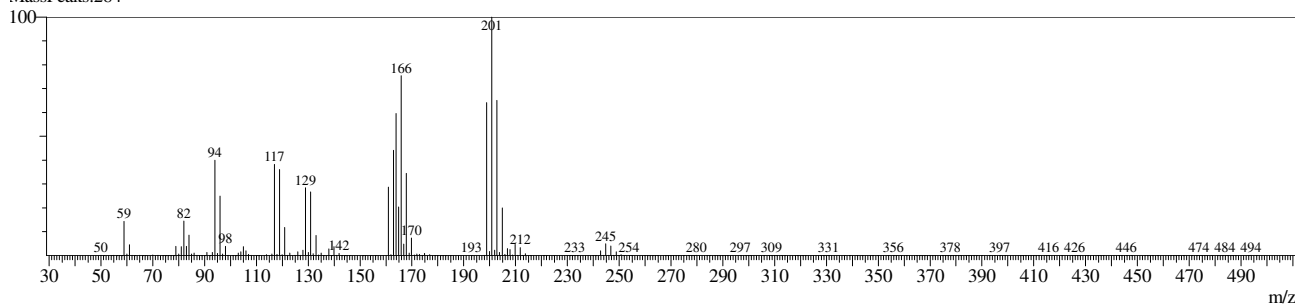

Peak#:2 R.Time:7.295(Scan#:840)

MassPeaks:344

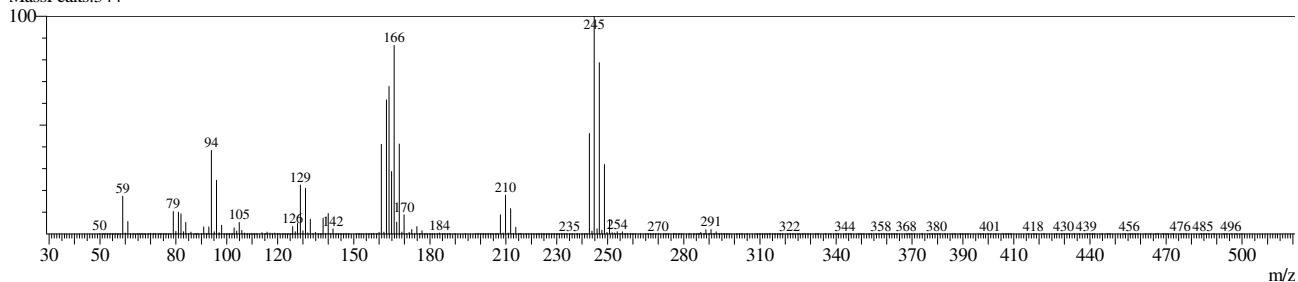

==== Analytical Line 1 =====

Split Ratio

Linear Velocity 36.3

Column Flow 1.00

Oven Temp. Program

Rate	Temperature(°C)	Hold Time(min)
-	50.0	2.00
25.00	250.0	8.00

--Group 1 - Event 1--

Start Time :3.10min
 End Time :17.00min
 ACQ Mode :Scan
 Event Time :0.30sec
 Scan Speed :1666
 Start m/z :50.00
 End m/z :500.00